


Client report

	No of participants	No of responded participants	Response percentage
Chlamydia pneumoniae, antibodies, June, 2-2024	42	39	92.9 %

Summary Result 1

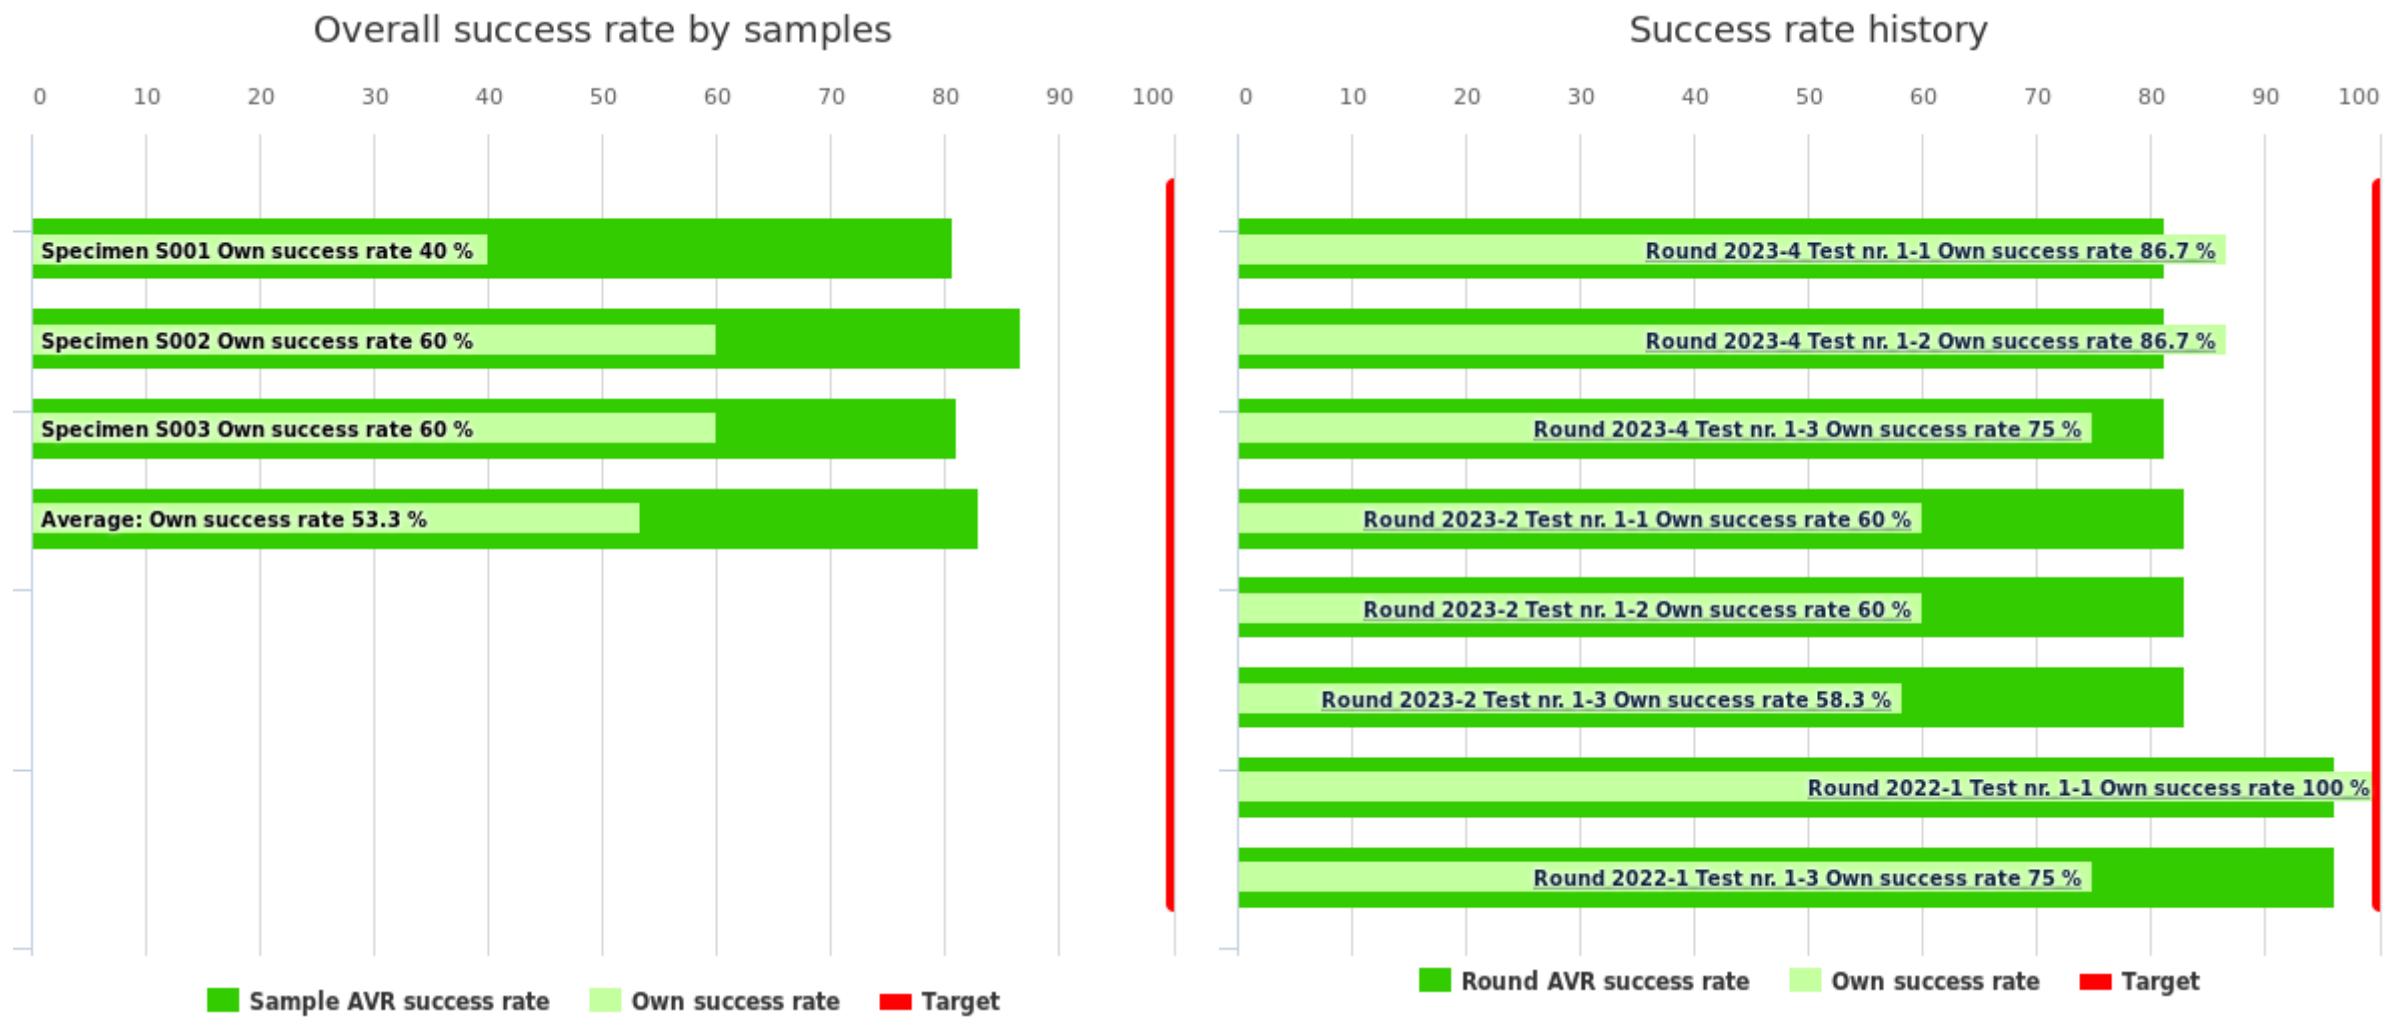


Summary	Own score	Max score	Own success rate	Difference	AVR success rate
Specimen S001	4	10	40 %	-40.7 %	80.7 %
Specimen S002	6	10	60 %	-26.7 %	86.7 %
Specimen S003	6	10	60 %	-21.1 %	81.1 %
Average:			53.3 %	-29.5 %	82.9 %

History	Test nr.	Own success rate	Difference	AVR success rate
Round 2023-4	1-1	86.7 %	5.4 %	81.3 %
Round 2023-4	1-2	86.7 %	5.4 %	81.3 %
Round 2023-4	1-3	75 %	-6.3 %	81.3 %
Round 2023-2	1-1	60 %	-23 %	83 %
Round 2023-2	1-2	60 %	-23 %	83 %
Round 2023-2	1-3	58.3 %	-24.7 %	83 %
Round 2022-1	1-1	100 %	3.8 %	96.2 %
Round 2022-1	1-3	75 %	-21.2 %	96.2 %


Specimen S001 Result 1

Specimen S001 success rate




Specimen S001 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-70 %	70 %	43
	CpnAbG	0	2	0 %	-69.8 %	69.8 %	43
	CpnAbM	2	2	100 %	0 %	100 %	41
	CpnAbA	2	2	100 %	4.5 %	95.5 %	22
	Total:	4	10	40 %	-40.7 %	80.7 %	149

Specimen S001 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	No detectable C. pneumoniae antibodies		21		-				100 %
	Most likely earlier infection/serological scar	A second sample is requested	9	3	0	4	0 %	0 %	0 %
		A second sample is requested		3	-	-			
	Laboratory does not give clinical interpretation		13		-				-
		A second sample is requested		1	-	-			
	Total:		43		0	4	0 %	-70 %	70 %


Specimen S001 CpnAbG

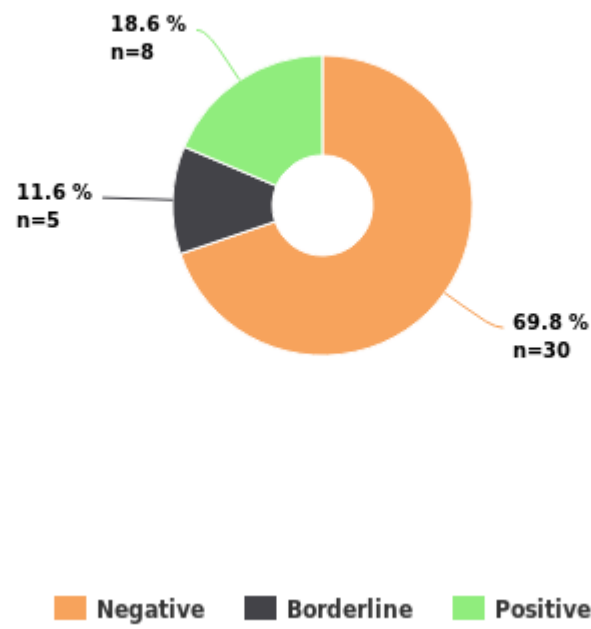

Specimen S001 CpnAbM



Specimen S001 CpnAbA



OWN DEVICE: SUNRISE

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		30		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		2					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		4					
		Siemens Novagnost		1					
		Vircell Chlamydoiphila pneumoniae ELISA		3					
		Vircell Chlamydoiphila pneumoniae IFA		1					
		Vircell Chlamydoiphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Borderline		5		-				0 %
		Labsystems Diagnostics Chlamydia pneumoniae EIA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
		Vircell Chlamydoiphila pneumoniae VIRCLIA Monotest		1					
	Positive		8		0	2	0 %	0 %	0 %

	Novatec NovaLisa C. pneumoniae ELISA		2						
	Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		1						
	Savyon Diagnostics SeroCP Quant kit		1						
	TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1						
	<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1						
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1						
	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1						
	Total:		43		0	2	0 %	-69.8 %	69.8 %

OWN DEVICE: SUNRISE


CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		41		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		2	2	100 %	0 %	100 %

OWN DEVICE: SUNRISE

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		21		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		6					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		2					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	Borderline		1		-				0 %
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
	Total:		22		2	2	100 %	4.5 %	95.5 %


Specimen S002 Result 1

Specimen S002 success rate




Specimen S002 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-76.7 %	76.7 %	43
	CpnAbG	2	2	100 %	0 %	100 %	43
	CpnAbM	2	2	100 %	0 %	100 %	41
	CpnAbA	2	2	100 %	36.4 %	63.6 %	22
	Total:	6	10	60 %	-26.7 %	86.7 %	149

Specimen S002 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Most likely acute/recent C. pneumoniae infection		7		0	4	0 %	0 %	0 %
		A second sample is requested		1	-	-			
		Referred to confirmation		1	-	-			
	Most likely earlier infection/serological scar		23		-	-			100 %
		A second sample is requested		5	-	-			
	Laboratory does not give clinical interpretation		13		-	-			-
		A second sample is requested		1	-	-			
	Total:		43		0	4	0 %	-76.7 %	76.7 %

Specimen S002 CpnAbG




Positive

Specimen S002 CpnAbM



Negative

Specimen S002 CpnAbA



Negative Borderline Positive

OWN DEVICE: SUNRISE

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Positive		43		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP Quant kit		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					
	<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae			1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydothila pneumoniae ELISA		3					
		Vircell Chlamydothila pneumoniae IFA		1					
		Vircell Chlamydothila pneumoniae VIRCLIA Monotest		4					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		43		2	2	100 %	0 %	100 %

OWN DEVICE: SUNRISE


CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		41		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		2	2	100 %	0 %	100 %

OWN DEVICE: SUNRISE

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		8		-				0 %
		Euroimmun Anti-C. pneumoniae ELISA		5					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
	Borderline		1		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		1					
	<input checked="" type="radio"/> Positive		13		2	2	100 %	0 %	100 %
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		2					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	Total:		22		2	2	100 %	36.4 %	63.6 %


Specimen S003 Result 1

Specimen S003 success rate




Specimen S003 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-69 %	69 %	43
	CpnAbG	2	2	100 %	16.3 %	83.7 %	43
	CpnAbM	2	2	100 %	0 %	100 %	41
	CpnAbA	2	2	100 %	27.3 %	72.7 %	22
	Total:	6	10	60 %	-21.1 %	81.1 %	149

Specimen S003 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	No detectable C. pneumoniae antibodies		4		-				0 %
		A second sample is requested		1	-	-			
	<input checked="" type="radio"/> Most likely acute/recent C. pneumoniae infection		5		0	4	0 %	0 %	0 %
	Most likely earlier infection/serological scar		20		-				100 %
		A second sample is requested		6	-	-			
	Laboratory does not give clinical interpretation		14		-				-
		A second sample is requested		2	-	-			
	Total:		43		0	4	0 %	-69 %	69 %

Specimen S003 CpnAbG




■ Negative
 ■ Borderline
 ■ Positive

Specimen S003 CpnAbM



■ Negative

Specimen S003 CpnAbA



■ Negative
 ■ Borderline
 ■ Positive

OWN DEVICE: SUNRISE

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		7		-				0 %
		Novatec NovaLisa C. pneumoniae ELISA		2					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		Vircell Chlamydomphila pneumoniae ELISA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		1					
	Borderline		9		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		1					
		Euroimmun Anti-Chlamydia pneumoniae MIF		1					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		1					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		4					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	<input checked="" type="radio"/> Positive		27		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		9					
		Euroimmun Anti-Chlamydia pneumoniae MIF		1					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		2					
		Savyon Diagnostics SeroCP Quant kit		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					

	<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1						
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1						
	TestLine Clinical Diagnostics Microblot-Array Chlamydia		1						
	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2						
	Vircell Chlamydomphila pneumoniae ELISA		2						
	Vircell Chlamydomphila pneumoniae IFA		1						
	Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3						
	Virion/Serion SERION ELISA classic C. pneumoniae		2						
	Total:		43		2	2	100 %	16.3 %	83.7 %

OWN DEVICE: SUNRISE

CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		41		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		2	2	100 %	0 %	100 %

OWN DEVICE: SUNRISE


CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		6		-				0 %
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
	Borderline		3		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		2					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	<input checked="" type="radio"/> Positive		13		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		4					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
		TestLine Clinical Diagnostics Microblot-Array Chlamydia		1					

		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
		Vircell Chlamydophila pneumoniae ELISA		2					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		3					
	Total:		22		2	2	100 %	27.3 %	72.7 %

Client report

	No of participants	No of responded participants	Response percentage
Chlamydia pneumoniae, antibodies, June, 2-2024	42	39	92.9 %

Summary Result 2

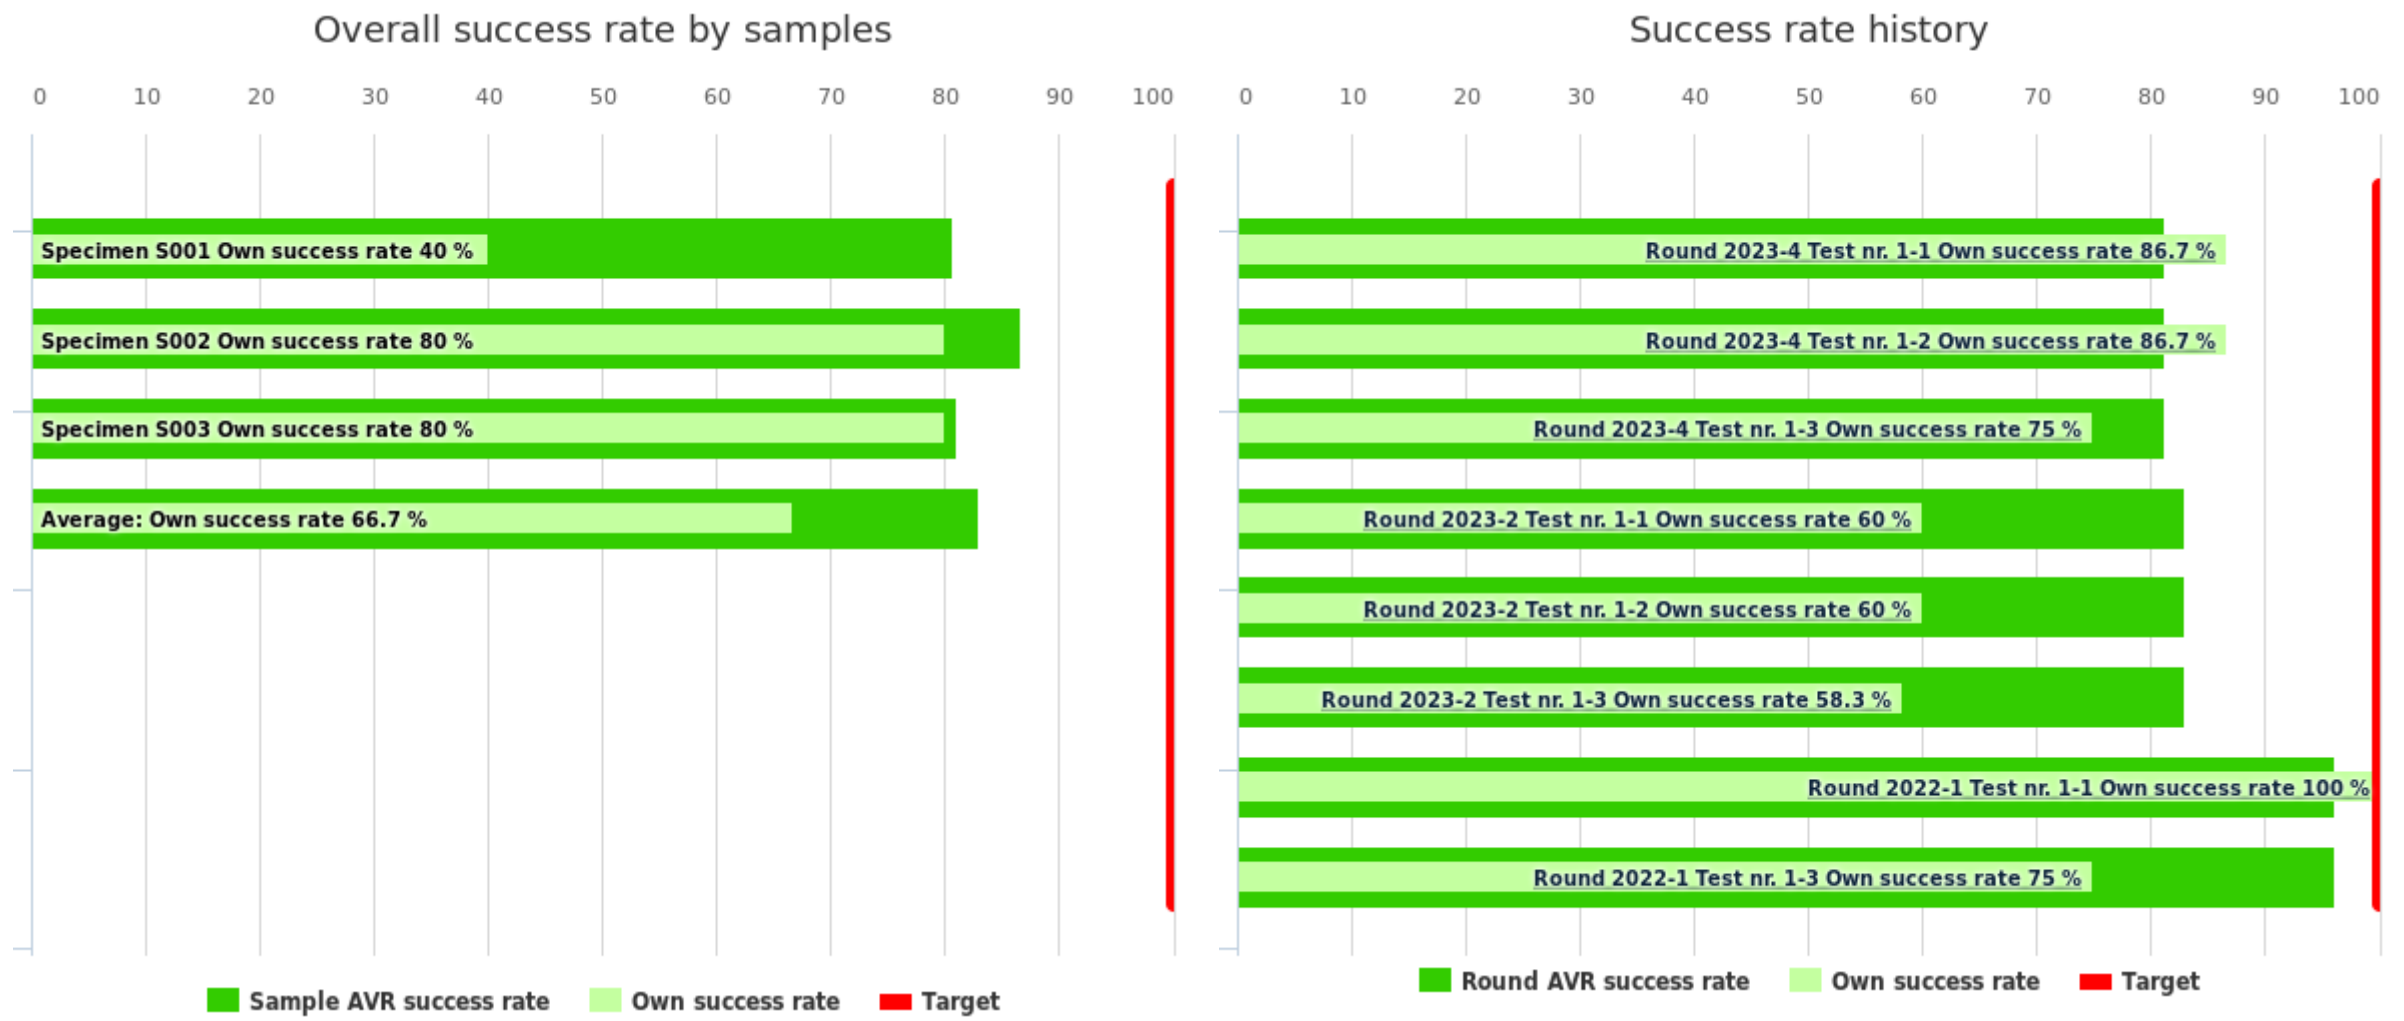


Summary	Own score	Max score	Own success rate	Difference	AVR success rate
Specimen S001	4	10	40 %	-40.7 %	80.7 %
Specimen S002	8	10	80 %	-6.7 %	86.7 %
Specimen S003	8	10	80 %	-1.1 %	81.1 %
Average:			66.7 %	-16.2 %	82.9 %

History	Test nr.	Own success rate	Difference	AVR success rate
Round 2023-4	1-1	86.7 %	5.4 %	81.3 %
Round 2023-4	1-2	86.7 %	5.4 %	81.3 %
Round 2023-4	1-3	75 %	-6.3 %	81.3 %
Round 2023-2	1-1	60 %	-23 %	83 %
Round 2023-2	1-2	60 %	-23 %	83 %
Round 2023-2	1-3	58.3 %	-24.7 %	83 %
Round 2022-1	1-1	100 %	3.8 %	96.2 %
Round 2022-1	1-3	75 %	-21.2 %	96.2 %


Specimen S001 Result 2

Specimen S001 success rate




Specimen S001 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-70 %	70 %	43
	CpnAbG	0	2	0 %	-69.8 %	69.8 %	43
	CpnAbM	2	2	100 %	0 %	100 %	41
	CpnAbA	2	2	100 %	4.5 %	95.5 %	22
	Total:	4	10	40 %	-40.7 %	80.7 %	149

Specimen S001 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	No detectable C. pneumoniae antibodies		21		-				100 %
	Most likely earlier infection/serological scar	A second sample is requested	9	3	0	4	0 %	0 %	0 %
		A second sample is requested		3	-	-			
	Laboratory does not give clinical interpretation		13		-				-
		A second sample is requested		1	-	-			
	Total:		43		0	4	0 %	-70 %	70 %


Specimen S001 CpnAbG

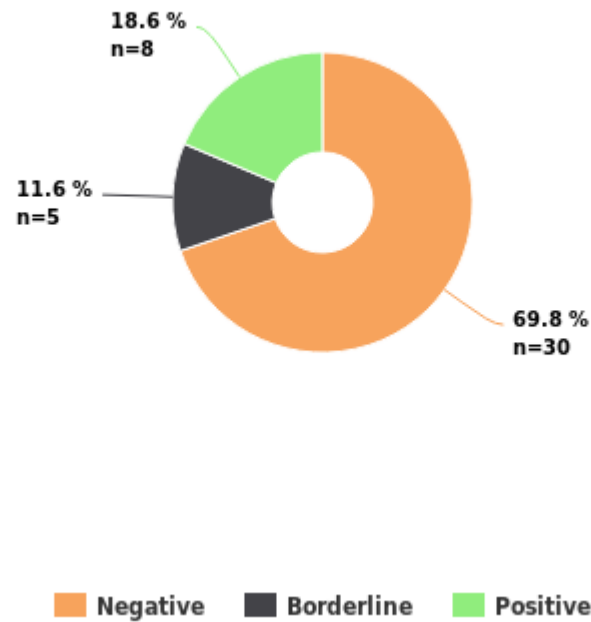

Specimen S001 CpnAbM



Specimen S001 CpnAbA



OWN DEVICE: KLEEYA

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		30		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		2					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		4					
		Siemens Novagnost		1					
		Vircell Chlamydophila pneumoniae ELISA		3					
		Vircell Chlamydophila pneumoniae IFA		1					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Borderline		5		0	2	0 %	0 %	0 %
		Labsystems Diagnostics Chlamydia pneumoniae EIA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		1					
	Positive		8		-				0 %

	Novatec NovaLisa C. pneumoniae ELISA		2						
	Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		1						
	Savyon Diagnostics SeroCP Quant kit		1						
	TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1						
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1						
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1						
	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1						
	Total:		43		0	2	0 %	-69.8 %	69.8 %

OWN DEVICE: KLEEYA


CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		41		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		2	2	100 %	0 %	100 %

OWN DEVICE: KLEEYA

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		21		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		6					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		2					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	Borderline		1		-				0 %
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
	Total:		22		2	2	100 %	4.5 %	95.5 %


Specimen S002 Result 2

Specimen S002 success rate




Specimen S002 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	4	4	100 %	23.3 %	76.7 %	43
	CpnAbG	2	2	100 %	0 %	100 %	43
	CpnAbM	2	2	100 %	0 %	100 %	41
	CpnAbA	0	2	0 %	-63.6 %	63.6 %	22
	Total:	8	10	80 %	-6.7 %	86.7 %	149

Specimen S002 Clinical interpretation

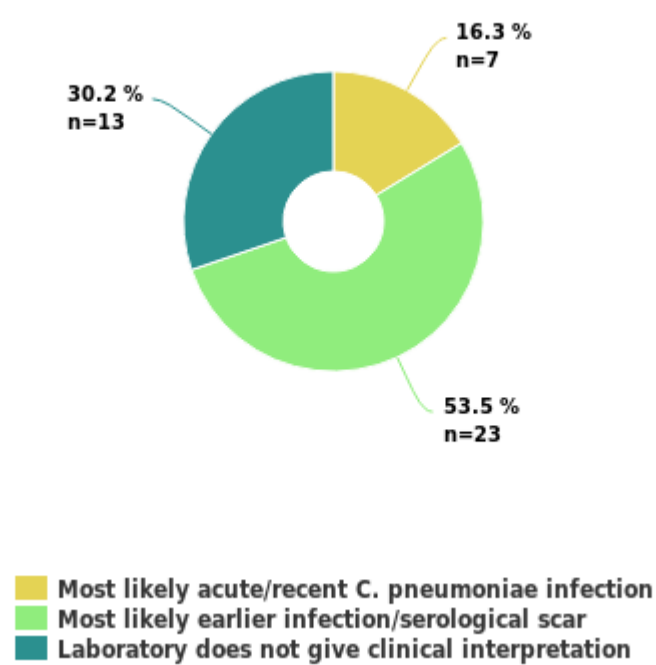


Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	Most likely acute/recent C. pneumoniae infection		7		-	-			0 %
		A second sample is requested		1	-	-			
		Referred to confirmation		1	-	-			
	<input checked="" type="radio"/> Most likely earlier infection/serological scar		23		4	4	100 %	0 %	100 %
		A second sample is requested		5	-	-			
	Laboratory does not give clinical interpretation		13		-	-			-
		A second sample is requested		1	-	-			
	Total:		43		4	4	100 %	23.3 %	76.7 %

Specimen S002 CpnAbG




Positive

Specimen S002 CpnAbM



Negative

Specimen S002 CpnAbA



Negative Borderline Positive

OWN DEVICE: KLEEYA

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Positive		43		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP Quant kit		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydothila pneumoniae ELISA		3					
		Vircell Chlamydothila pneumoniae IFA		1					
		Vircell Chlamydothila pneumoniae VIRCLIA Monotest		4					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		43		2	2	100 %	0 %	100 %

OWN DEVICE: KLEEYA


CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		41		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		2	2	100 %	0 %	100 %

OWN DEVICE: KLEEYA

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		8		0	2	0 %	0 %	0 %
		Euroimmun Anti-C. pneumoniae ELISA		5					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Siemens Novagnost		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
	Borderline		1		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		1					
	<input checked="" type="radio"/> Positive		13		-				100 %
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		2					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	Total:		22		0	2	0 %	-63.6 %	63.6 %


Specimen S003 Result 2

Specimen S003 success rate




Specimen S003 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	4	4	100 %	31 %	69 %	43
	CpnAbG	2	2	100 %	16.3 %	83.7 %	43
	CpnAbM	2	2	100 %	0 %	100 %	41
	CpnAbA	0	2	0 %	-72.7 %	72.7 %	22
	Total:	8	10	80 %	-1.1 %	81.1 %	149

Specimen S003 Clinical interpretation

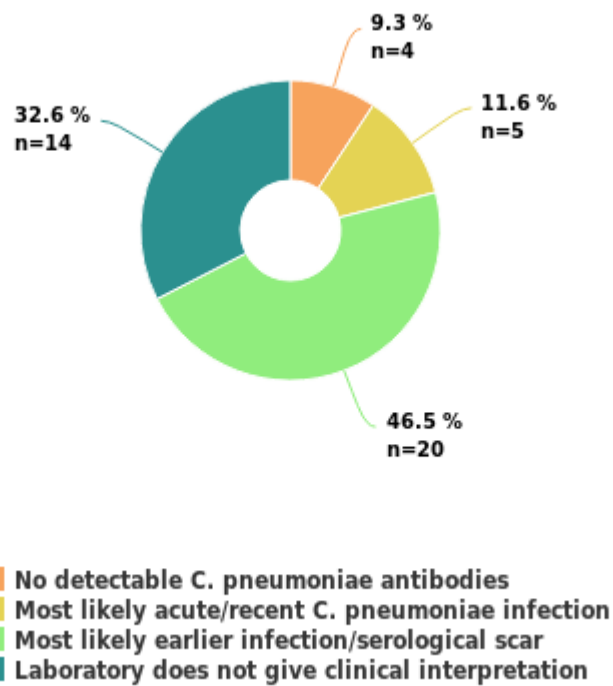


Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	No detectable C. pneumoniae antibodies		4		-				0 %
		A second sample is requested		1	-	-			
	Most likely acute/recent C. pneumoniae infection		5		-				0 %
	<input checked="" type="radio"/> Most likely earlier infection/serological scar		20		4	4	100 %	0 %	100 %
		A second sample is requested		6	-	-			
	Laboratory does not give clinical interpretation		14		-				-
		A second sample is requested		2	-	-			
	Total:		43		4	4	100 %	31 %	69 %

Specimen S003 CpnAbG




■ Negative
 ■ Borderline
 ■ Positive

Specimen S003 CpnAbM



■ Negative

Specimen S003 CpnAbA



■ Negative
 ■ Borderline
 ■ Positive

OWN DEVICE: KLEEYA

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		7		-				0 %
		Novatec NovaLisa C. pneumoniae ELISA		2					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		Vircell Chlamydothila pneumoniae ELISA		1					
		Vircell Chlamydothila pneumoniae VIRCLIA Monotest		1					
	Borderline		9		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		1					
		Euroimmun Anti-Chlamydia pneumoniae MIF		1					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		1					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		4					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	<input checked="" type="radio"/> Positive		27		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		9					
		Euroimmun Anti-Chlamydia pneumoniae MIF		1					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		2					
		Savyon Diagnostics SeroCP Quant kit		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					

	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1						
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1						
	TestLine Clinical Diagnostics Microblot-Array Chlamydia		1						
	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2						
	Vircell Chlamydomphila pneumoniae ELISA		2						
	Vircell Chlamydomphila pneumoniae IFA		1						
	Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3						
	Virion/Serion SERION ELISA classic C. pneumoniae		2						
	Total:		43		2	2	100 %	16.3 %	83.7 %

OWN DEVICE: KLEEYA

CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		41		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		2	2	100 %	0 %	100 %

OWN DEVICE: KLEEYA


CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		6		0	2	0 %	0 %	0 %
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
	Borderline		3		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		2					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	<input checked="" type="radio"/> Positive		13		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		4					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
		TestLine Clinical Diagnostics Microblot-Array Chlamydia		1					

	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
	Vircell Chlamydophila pneumoniae ELISA		2					
	Vircell Chlamydophila pneumoniae VIRCLIA Monotest		3					
	Total:		22	0	2	0 %	-72.7 %	72.7 %

Client report

	No of participants	No of responded participants	Response percentage
Chlamydia pneumoniae, antibodies, June, 2-2024	42	39	92.9 %

Summary Result 3

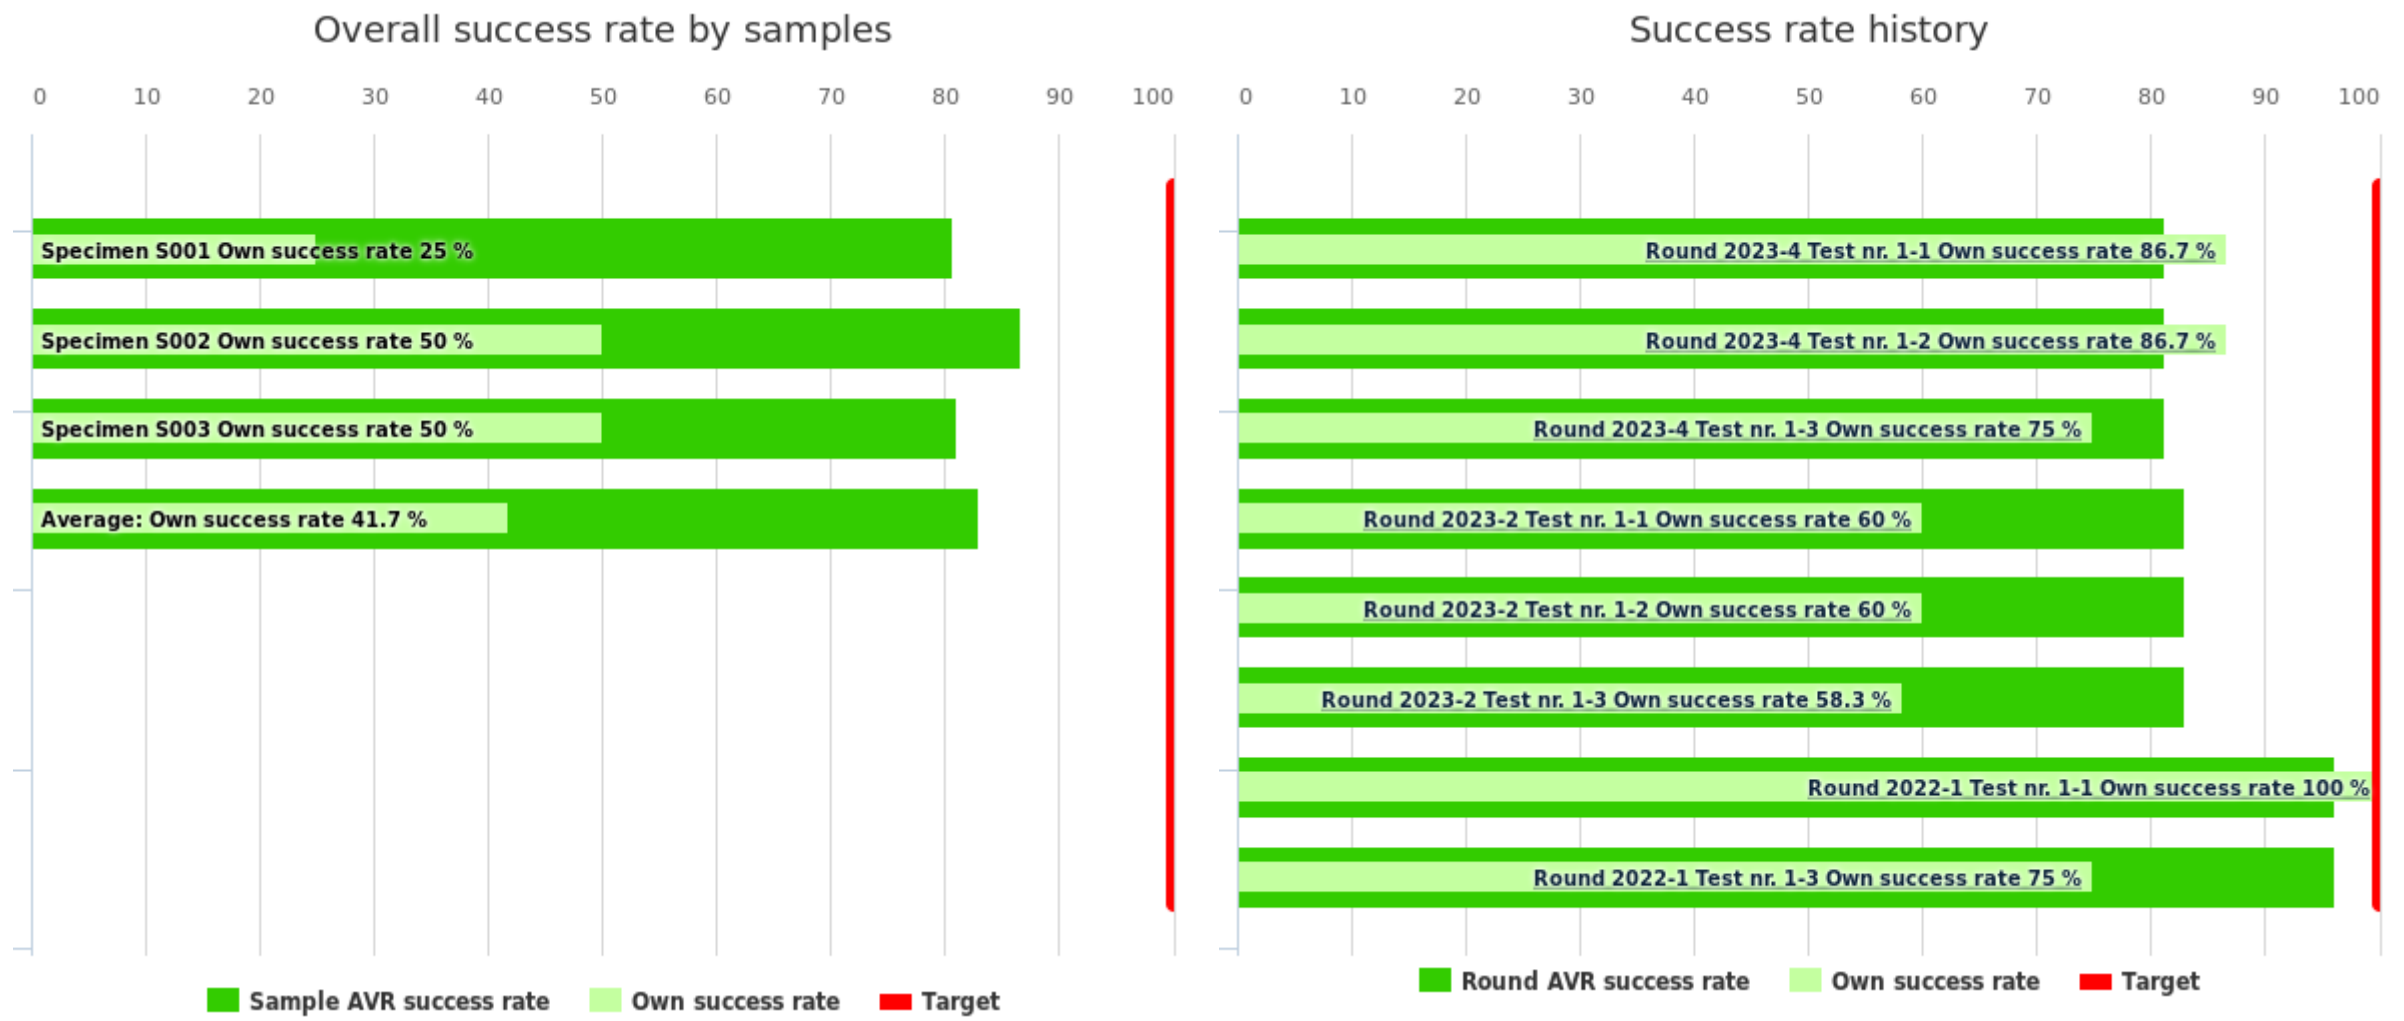


Summary	Own score	Max score	Own success rate	Difference	AVR success rate
Specimen S001	2	8	25 %	-55.7 %	80.7 %
Specimen S002	4	8	50 %	-36.7 %	86.7 %
Specimen S003	4	8	50 %	-31.1 %	81.1 %
Average:			41.7 %	-41.2 %	82.9 %

History	Test nr.	Own success rate	Difference	AVR success rate
Round 2023-4	1-1	86.7 %	5.4 %	81.3 %
Round 2023-4	1-2	86.7 %	5.4 %	81.3 %
Round 2023-4	1-3	75 %	-6.3 %	81.3 %
Round 2023-2	1-1	60 %	-23 %	83 %
Round 2023-2	1-2	60 %	-23 %	83 %
Round 2023-2	1-3	58.3 %	-24.7 %	83 %
Round 2022-1	1-1	100 %	3.8 %	96.2 %
Round 2022-1	1-3	75 %	-21.2 %	96.2 %


Specimen S001 Result 3

Specimen S001 success rate




Specimen S001 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-70 %	70 %	43
	CpnAbG	0	2	0 %	-69.8 %	69.8 %	43
	CpnAbM	-	-	-	-	100 %	41
	CpnAbA	2	2	100 %	4.5 %	95.5 %	22
	Total:	2	8	25 %	-55.7 %	80.7 %	149

Specimen S001 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	No detectable C. pneumoniae antibodies		21		-				100 %
	Most likely earlier infection/serological scar	A second sample is requested	9	3	0	4	0 %	0 %	0 %
		A second sample is requested		3	-	-			
	Laboratory does not give clinical interpretation		13		-				-
		A second sample is requested		1	-	-			
	Total:		43		0	4	0 %	-70 %	70 %


Specimen S001 CpnAbG



Specimen S001 CpnAbM



Specimen S001 CpnAbA



OWN DEVICE: AUTOBLOT 3000

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		30		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		2					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		4					
		Siemens Novagnost		1					
		Vircell Chlamydophila pneumoniae ELISA		3					
		Vircell Chlamydophila pneumoniae IFA		1					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Borderline		5		-				0 %
		Labsystems Diagnostics Chlamydia pneumoniae EIA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		1					
	Positive		8		0	2	0 %	0 %	0 %
		Novatec NovaLisa C. pneumoniae ELISA		2					

	Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs	1							
	Savyon Diagnostics SeroCP Quant kit	1							
	<input checked="" type="radio"/> TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae	1							
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae	1							
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG	1							
	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae	1							
	Total:	43	0	2	0 %	-69.8 %	69.8 %		


CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		41		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		-	-	-	-	100 %

OWN DEVICE: AUTOBLOT 3000

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Negative		21		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		6					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		2					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	Borderline		1		-				0 %
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
	Total:		22		2	2	100 %	4.5 %	95.5 %


Specimen S002 Result 3

Specimen S002 success rate




Specimen S002 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-76.7 %	76.7 %	43
	CpnAbG	2	2	100 %	0 %	100 %	43
	CpnAbM	-	-	-	-	100 %	41
	CpnAbA	2	2	100 %	36.4 %	63.6 %	22
	Total:	4	8	50 %	-36.7 %	86.7 %	149

Specimen S002 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Most likely acute/recent C. pneumoniae infection		7		0	4	0 %	0 %	0 %
		A second sample is requested		1	-	-			
		Referred to confirmation		1	-	-			
	Most likely earlier infection/serological scar		23		-	-			100 %
		A second sample is requested		5	-	-			
	Laboratory does not give clinical interpretation		13		-	-			-
		A second sample is requested		1	-	-			
	Total:		43		0	4	0 %	-76.7 %	76.7 %

Specimen S002 CpnAbG




Positive

Specimen S002 CpnAbM



Negative

Specimen S002 CpnAbA



Negative Borderline Positive

OWN DEVICE: AUTOBLOT 3000

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	<input checked="" type="radio"/> Positive		43		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP Quant kit		1					
		Siemens Novagnost		1					
	<input checked="" type="radio"/> TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae			1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydothila pneumoniae ELISA		3					
		Vircell Chlamydothila pneumoniae IFA		1					
		Vircell Chlamydothila pneumoniae VIRCLIA Monotest		4					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		43		2	2	100 %	0 %	100 %


CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		41		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		-	-	-	-	100 %

OWN DEVICE: AUTOBLOT 3000

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		8		-				0 %
		Euroimmun Anti-C. pneumoniae ELISA		5					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
	Borderline		1		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		1					
	<input checked="" type="radio"/> Positive		13		2	2	100 %	0 %	100 %
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics BLOT-LINE Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		2					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	Total:		22		2	2	100 %	36.4 %	63.6 %


Specimen S003 Result 3

Specimen S003 success rate




Specimen S003 results	Responded	Own score	Max score	Own success rate	Difference	AVR success rate	Count
	Clinical interpretation	0	4	0 %	-69 %	69 %	43
	CpnAbG	2	2	100 %	16.3 %	83.7 %	43
	CpnAbM	-	-	-	-	100 %	41
	CpnAbA	2	2	100 %	27.3 %	72.7 %	22
	Total:	4	8	50 %	-31.1 %	81.1 %	149

Specimen S003 Clinical interpretation




Clinical interpretation	Clinical interpretation	Further handling	Clinical interpretation count	Further handling count	Own score	Max score	Own success rate	Difference	AVR success rate
	No detectable C. pneumoniae antibodies		4		-				0 %
		A second sample is requested		1	-	-			
	<input checked="" type="radio"/> Most likely acute/recent C. pneumoniae infection		5		0	4	0 %	0 %	0 %
	Most likely earlier infection/serological scar		20		-				100 %
		A second sample is requested		6	-	-			
	Laboratory does not give clinical interpretation		14		-				-
		A second sample is requested		2	-	-			
	Total:		43		0	4	0 %	-69 %	69 %

Specimen S003 CpnAbG




■ Negative
 ■ Borderline
 ■ Positive

Specimen S003 CpnAbM



■ Negative

Specimen S003 CpnAbA



■ Negative
 ■ Borderline
 ■ Positive

OWN DEVICE: MICROBLLOT-ARRAY

CpnAbG	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		7		-				0 %
		Novatec NovaLisa C. pneumoniae ELISA		2					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		Vircell Chlamydophila pneumoniae ELISA		1					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		1					
	Borderline		9		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		1					
		Euroimmun Anti-Chlamydia pneumoniae MIF		1					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		1					
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		4					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	<input checked="" type="radio"/> Positive		27		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		9					
		Euroimmun Anti-Chlamydia pneumoniae MIF		1					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		2					
		Savyon Diagnostics SeroCP Quant kit		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgG		1					

	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1						
	TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgG		1						
	<input checked="" type="radio"/> TestLine Clinical Diagnostics Microblot-Array Chlamydia		1						
	TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2						
	Vircell Chlamydomphila pneumoniae ELISA		2						
	Vircell Chlamydomphila pneumoniae IFA		1						
	Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3						
	Virion/Serion SERION ELISA classic C. pneumoniae		2						
	Total:		43		2	2	100 %	16.3 %	83.7 %

CpnAbM	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		41		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		10					
		Euroimmun Anti-Chlamydia pneumoniae MIF		2					
		Labsystems Diagnostics Chlamydia pneumoniae EIA		3					
		Novatec NovaLisa C. pneumoniae ELISA		3					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		6					
		Savyon Diagnostics SeroCP		1					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgM		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		2					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		2					
		Vircell Chlamydomphila pneumoniae ELISA		3					
		Vircell Chlamydomphila pneumoniae IFA		1					
		Vircell Chlamydomphila pneumoniae VIRCLIA Monotest		3					
		Virion/Serion SERION ELISA classic C. pneumoniae		3					
	Total:		41		-	-	-	-	100 %

OWN DEVICE: MICROBLOT-ARRAY

CpnAbA	Result	Methodics	Result count	Methodics count	Own score	Max score	Own success rate	Difference	AVR success rate
	Negative		6		-				0 %
		Novatec NovaLisa C. pneumoniae ELISA		1					
		Orgentec Diagnostika Anti-Chlamydia pneumoniae Abs		2					
		Siemens Novagnost		1					
		TestLine Clinical Diagnostics CLIA Chlamydia pneumoniae IgA		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					
	Borderline		3		-				100 %
		Euroimmun Anti-C. pneumoniae ELISA		2					
		Virion/Serion SERION ELISA classic C. pneumoniae		1					
	<input checked="" type="radio"/> Positive		13		2	2	100 %	0 %	100 %
		Euroimmun Anti-C. pneumoniae ELISA		4					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae		1					
		TestLine Clinical Diagnostics EIA Chlamydia pneumoniae REC IgA		1					
		<input checked="" type="radio"/> TestLine Clinical Diagnostics Microblot-Array Chlamydia		1					
		TestLine Clinical Diagnostics SmartEIA Chlamydia pneumoniae		1					

		Vircell Chlamydophila pneumoniae ELISA		2					
		Vircell Chlamydophila pneumoniae VIRCLIA Monotest		3					
	Total:		22		2	2	100 %	27.3 %	72.7 %

Report Info**PARTICIPANTS**

Altogether 42 laboratories from 17 countries participated in this EQA round.

REPORT INFO

The results are divided into groups according to the method stated by the laboratory and presented in laboratory-specific tables. Accepted results are marked with green color and laboratory's own result with a black radio button . In the scoring report you will find summaries of overall success rate and sample specific success rates (%). Sample specific interpretations are shown in pie diagrams as percentages and the total interpretation and methodic counts in the tables. If you have not reported any results you will get a note: "You have not responded in time, only global report is available."

For information on report interpretation and performance evaluation, please see the "EQAS Interpretation guidelines" in LabScala User instructions. In case you have any questions regarding the reports, please contact the EQA Coordinator.

SCORING

The round is scored based on test results and clinical interpretations when 60% or more of the participants report the expected result and when at least three results are reported. The following general rules are applied:

Correct/expected test result 2/2 points
False/deviating test result 0/2 points
Correct/expected clinical interpretation 4/4 points
False/deviating clinical interpretation 0/4 points

The performance of the laboratory is assessed by the Own success rate (%). The target is 100%. The examination-specific scores obtained by the laboratory in the round are converted to Own success rate per sample (scores/maximum scores*100). The Laboratory's Own success rate is the average of the sample success rates. The success rate for the entire round (AVR success rate) is calculated from the total number of scores given to the results per sample (all scores/maximum scores*100). The AVG success rate of the entire round is the average of the sample success rates. The difference in the Laboratory's Own success rate (%) to the corresponding numbers for the entire round is shown in the table.